


### Product Selection Decision Tree

- Sample Risk Assessment Indicators:**
- Limited ability to reposition self
  - Braden score of 18 or less
  - Braden Activity subscore of 1-3
  - Braden Mobility subscore of 1 or 2
  - Braden Friction and Shear subscore of 1 or 2
  - Existing or history of pressure injuries

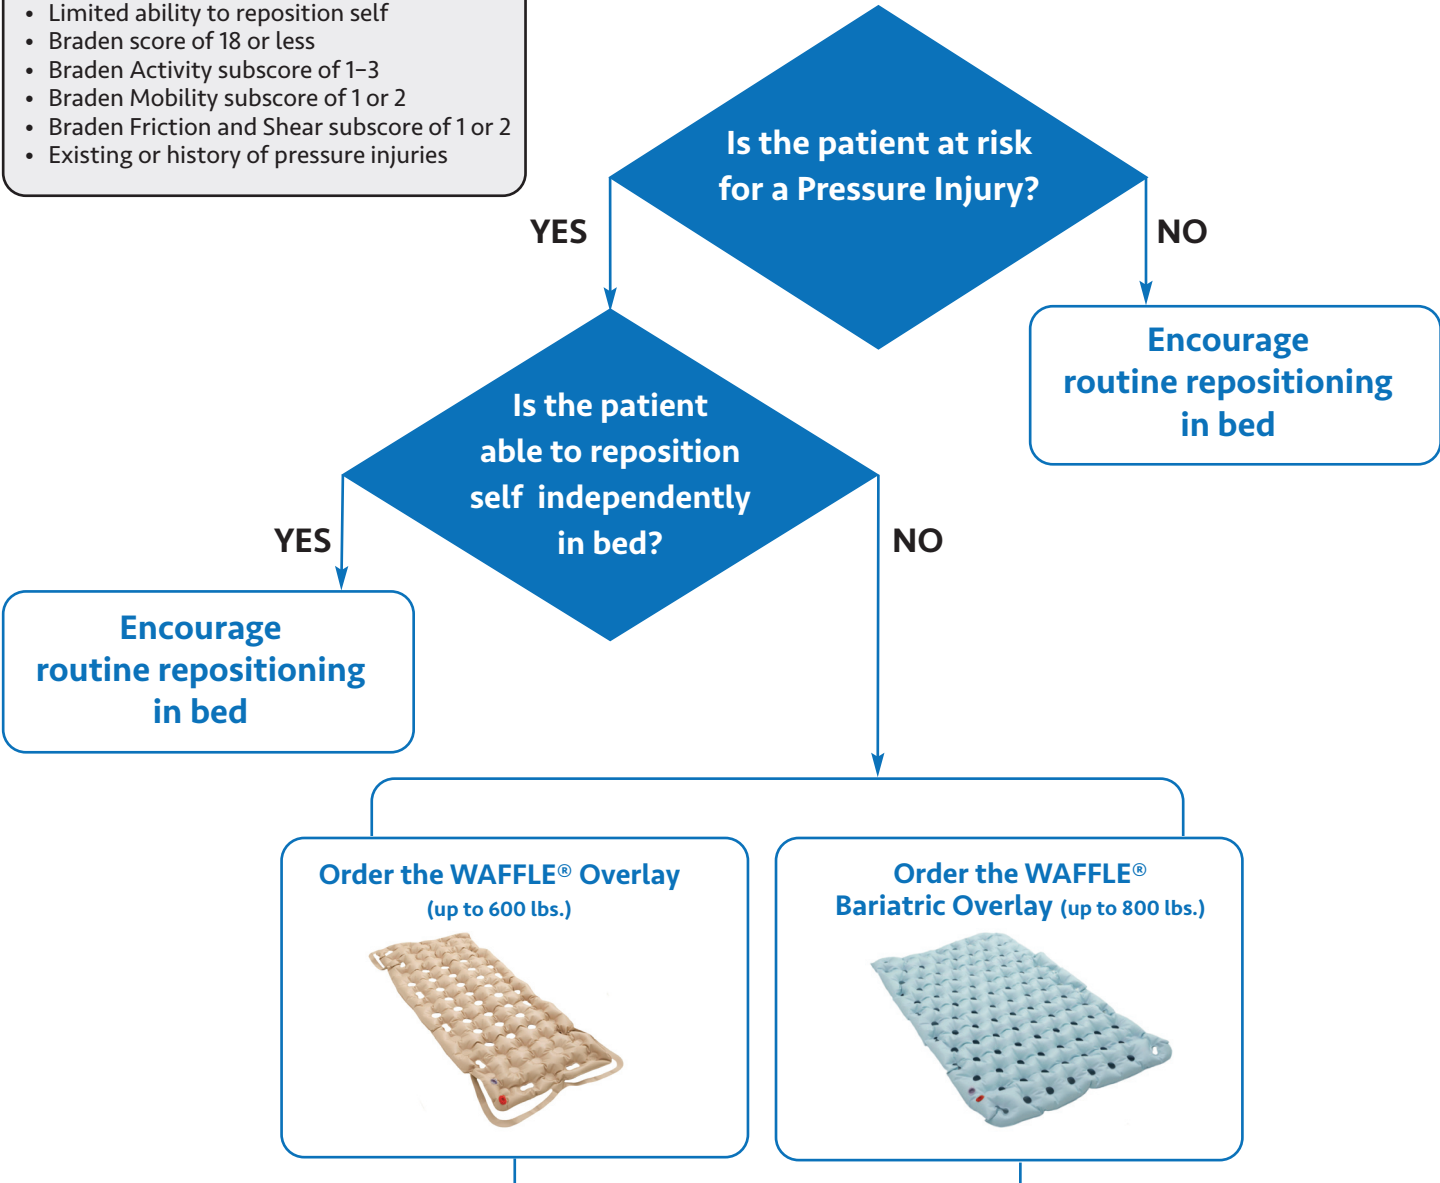

- Perform a hand check every shift and adjust inflation as needed
- Reposition the patient every 2 hours or per individualized repositioning schedule
- Use only one incontinence pad at a time
- Send WAFFLE Overlay with patient at discharge